

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**

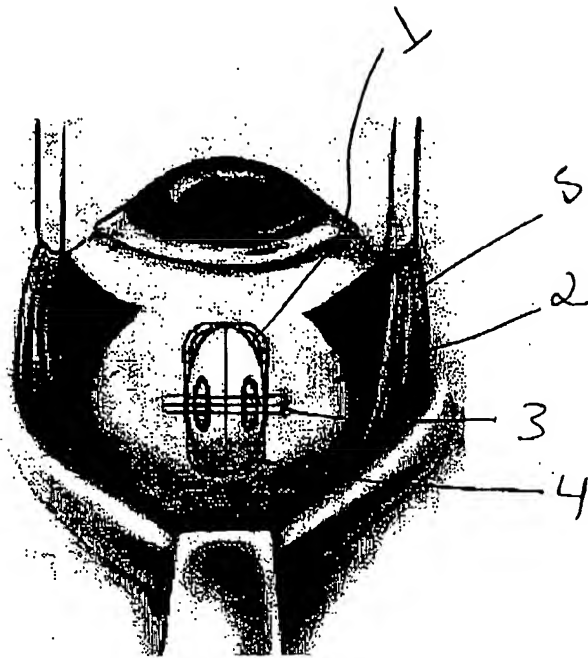


Fig. 1

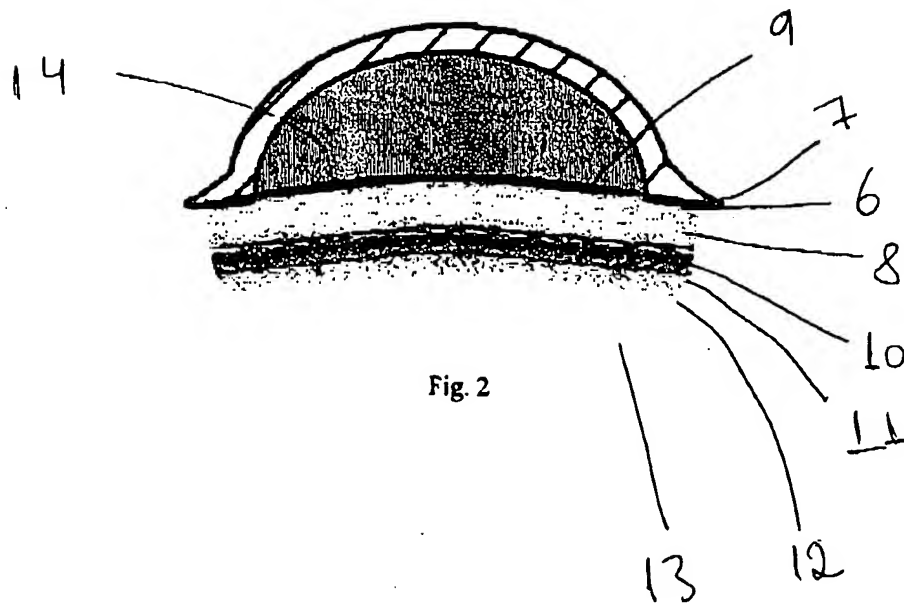


Fig. 2

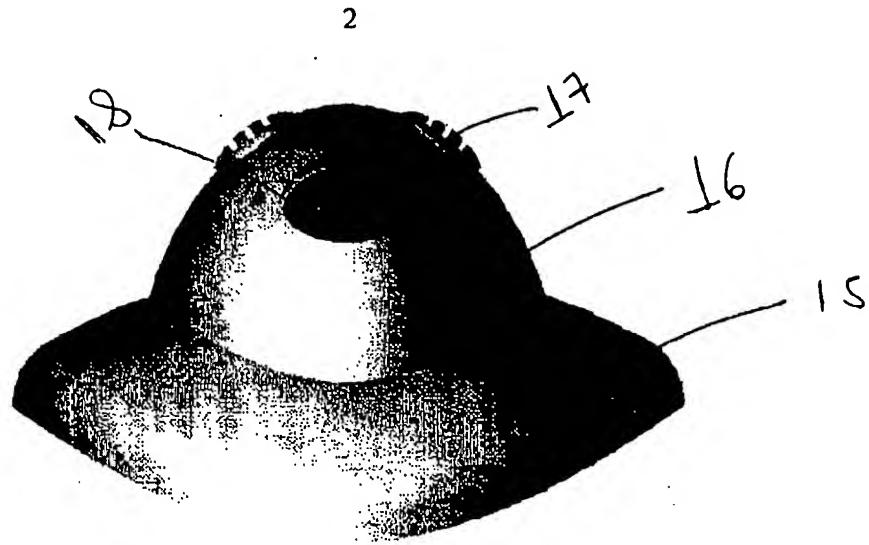


Fig. 3

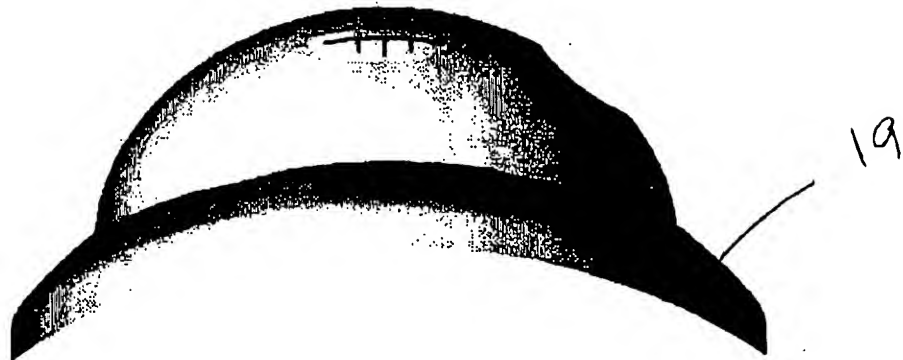


Fig. 4

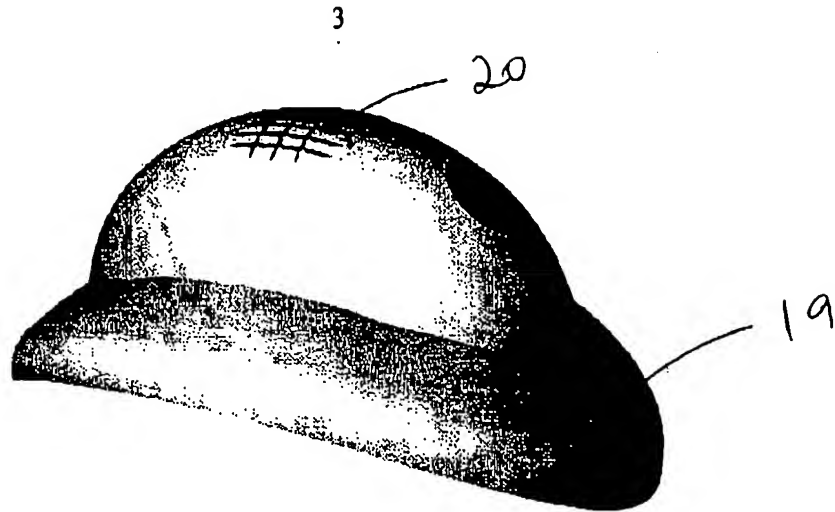


Fig. 5

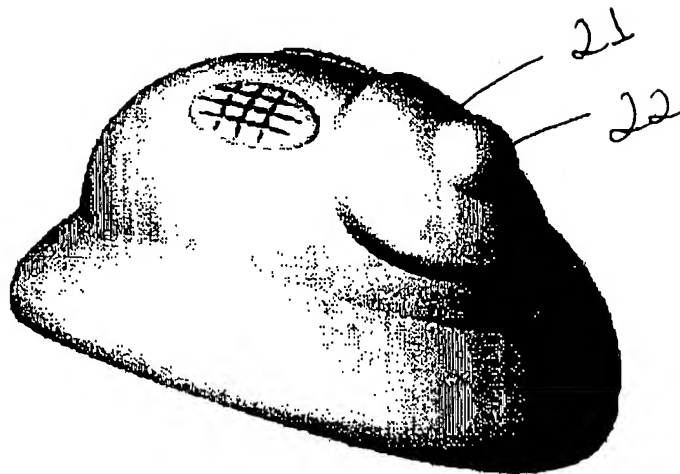


Fig. 6

4

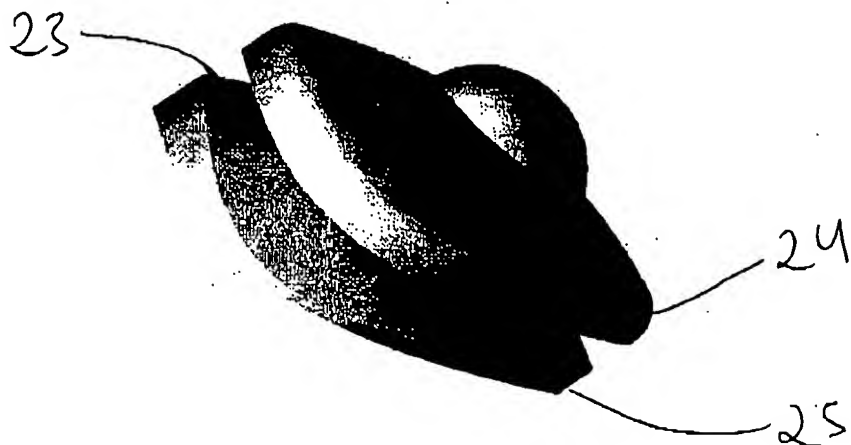


Fig. 7

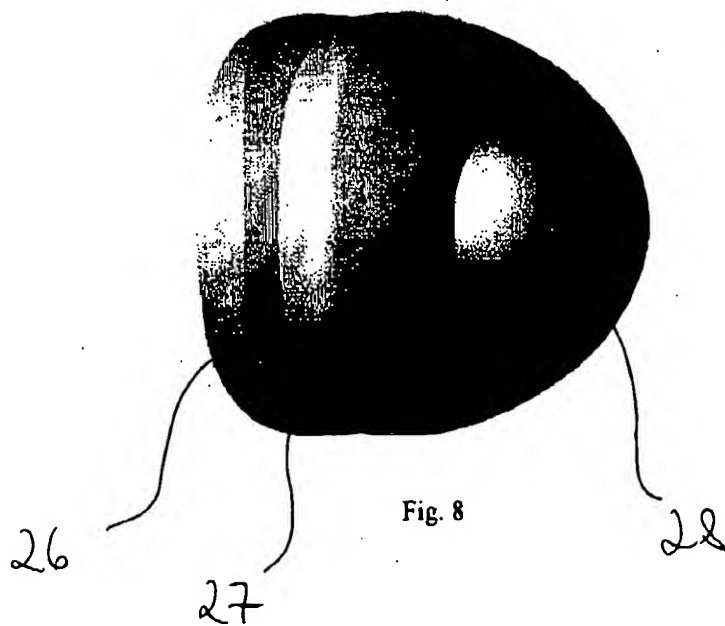


Fig. 8

4

5

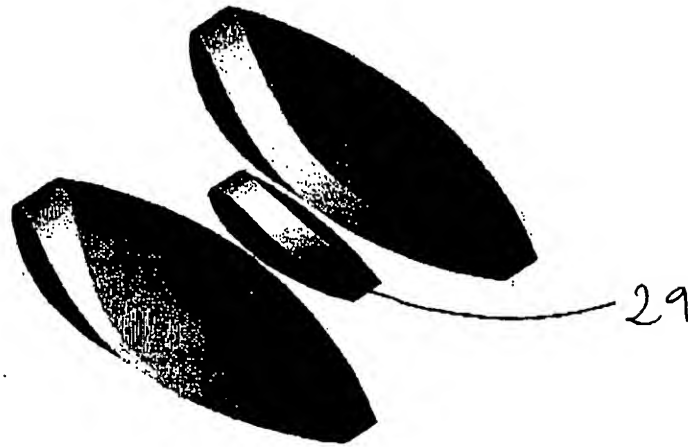


Fig. 9

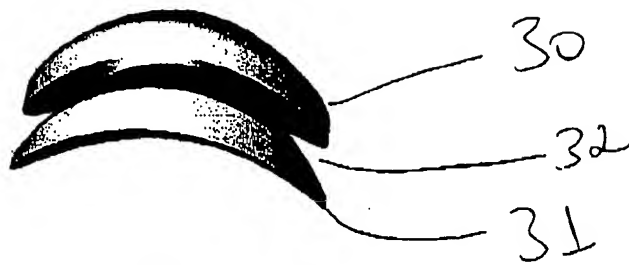


Fig. 10

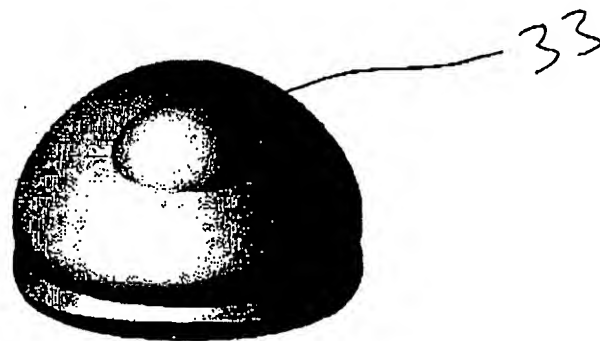


Fig. 11

5

6

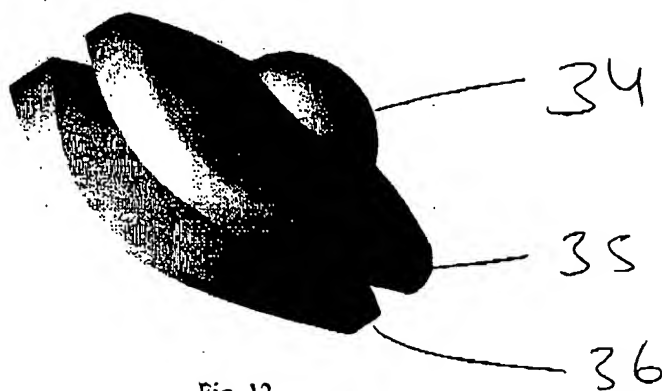


Fig. 12

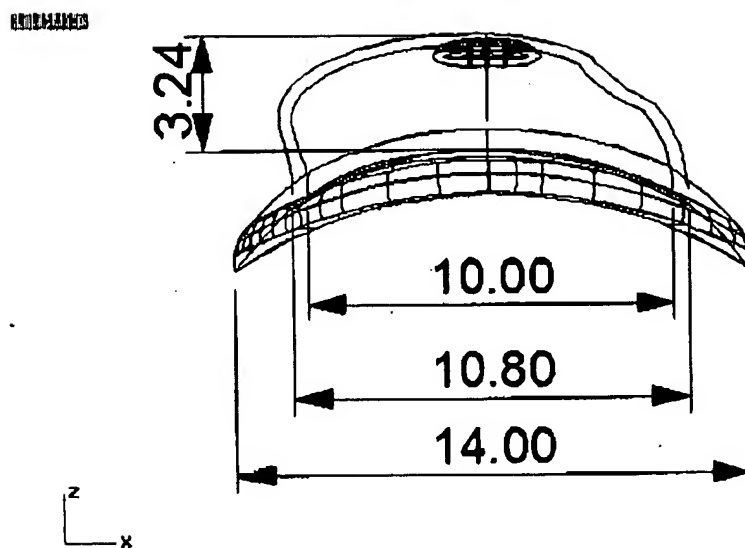


Fig. 13

7

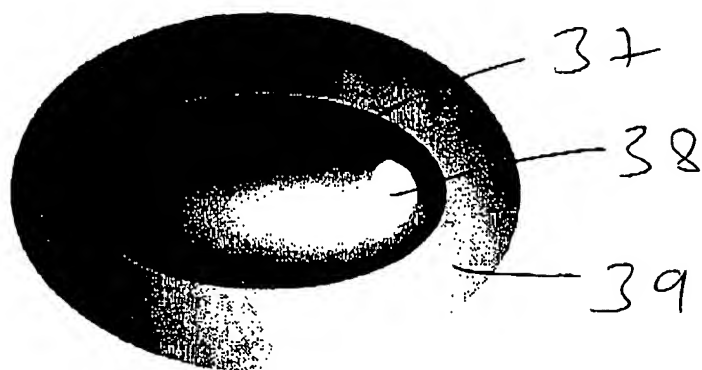


Fig. 14



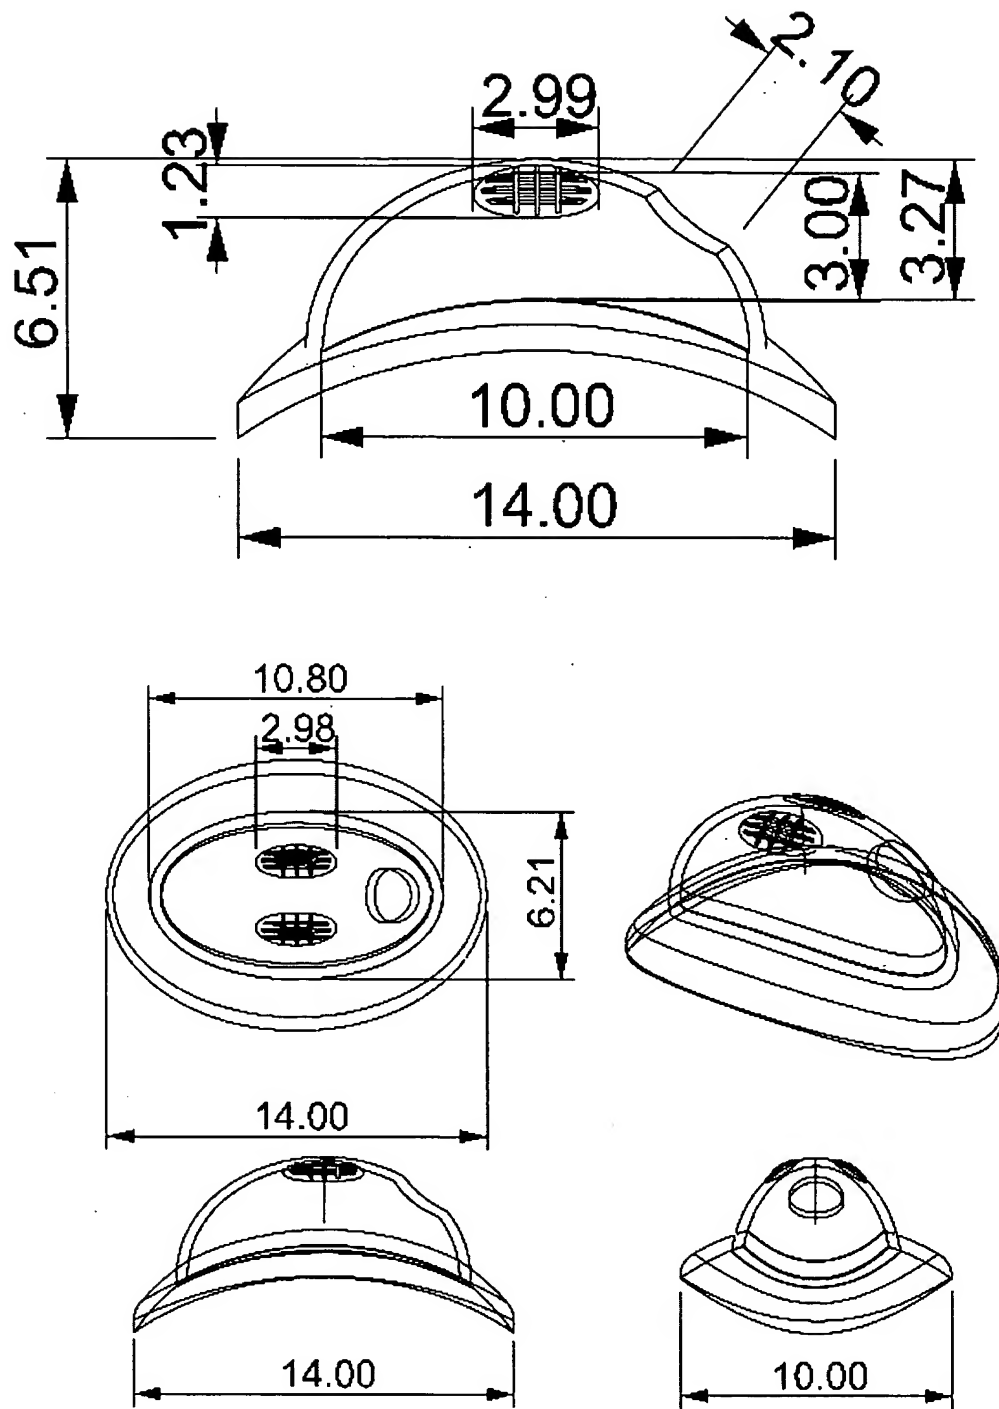


Fig. 15. Illustrative volume-oriented measures of the medical device.

9

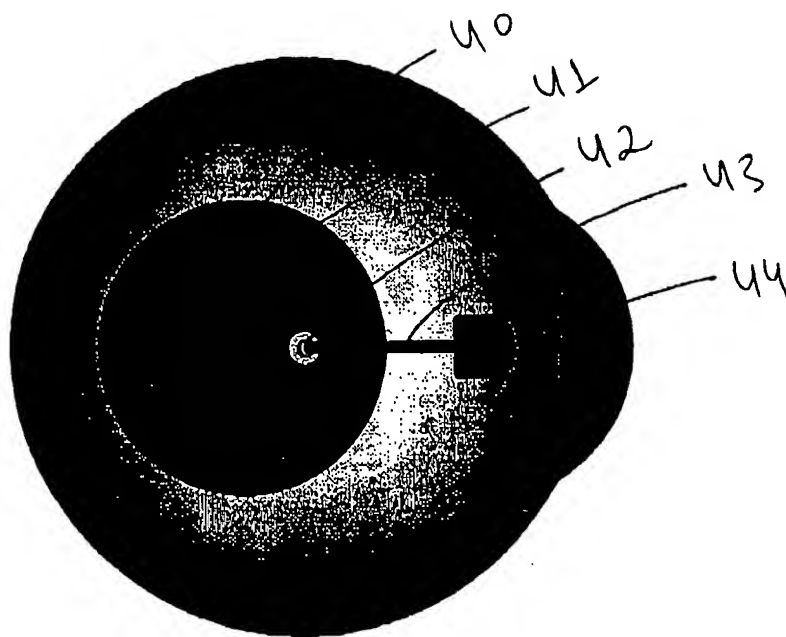


Fig. 16

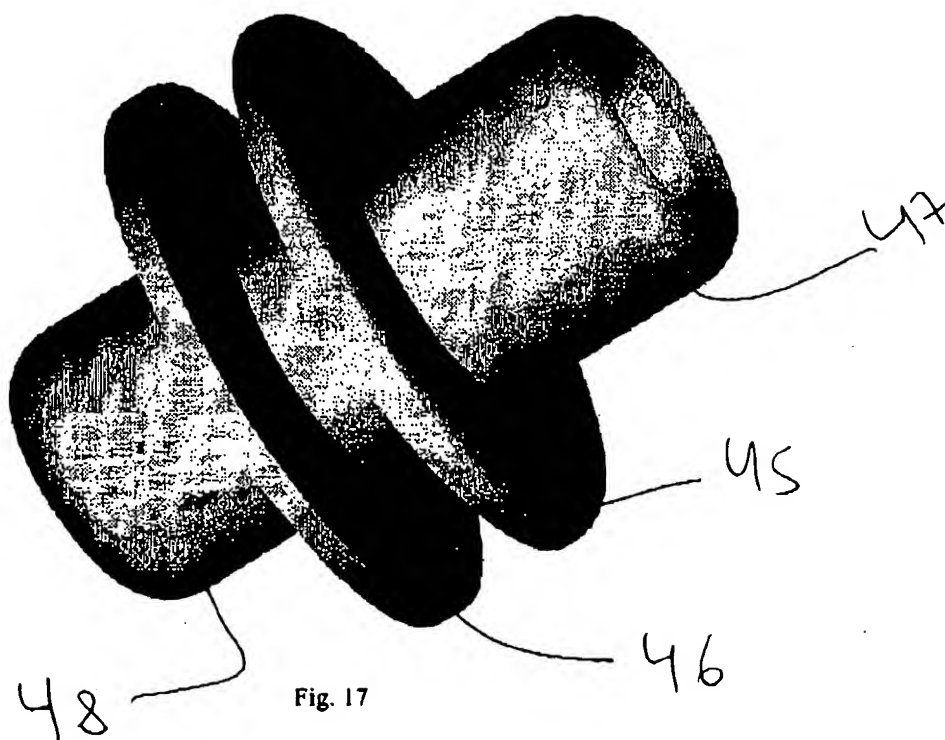


Fig. 17

9

10

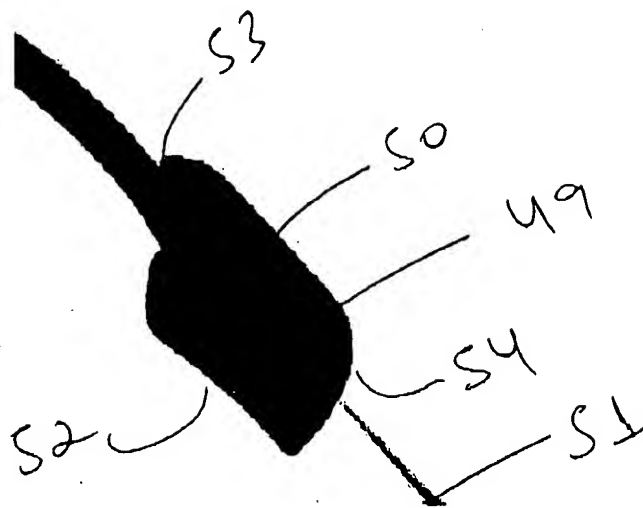


Fig. 18



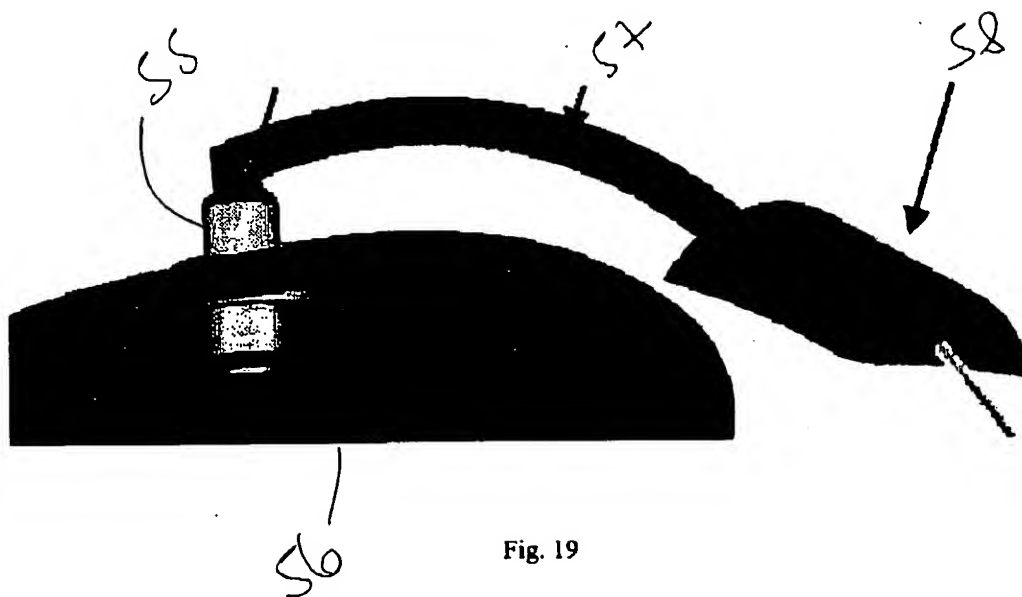


Fig. 19

10

11

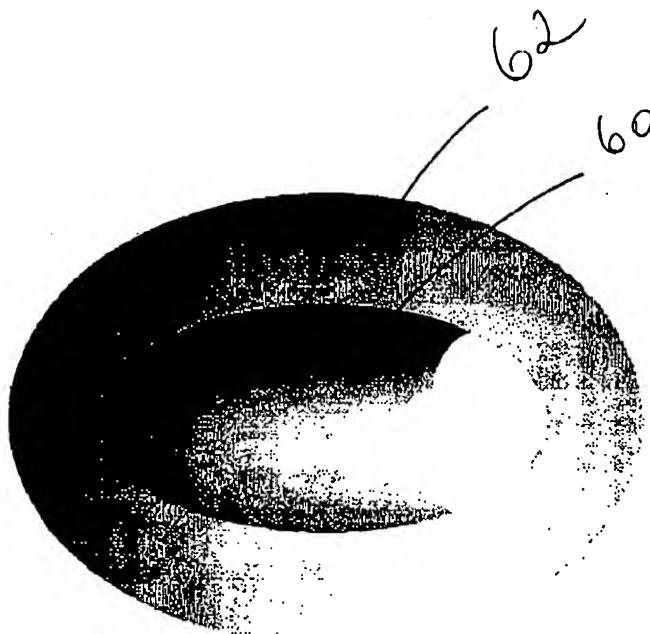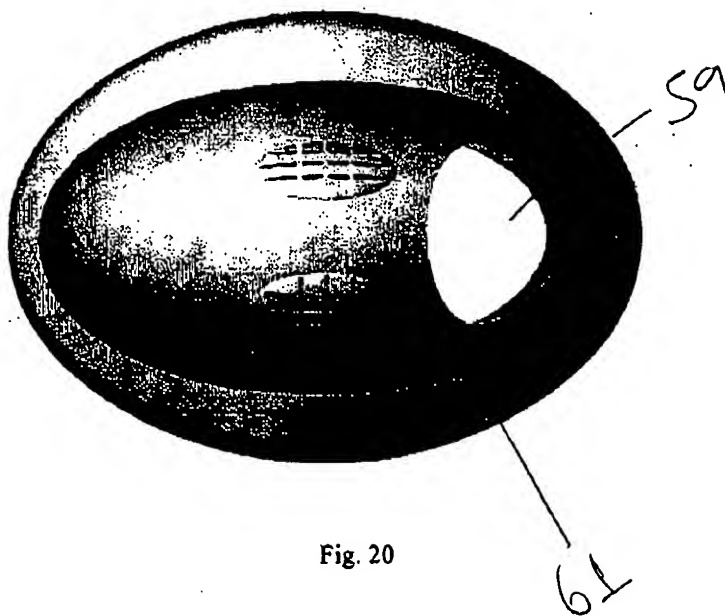

12

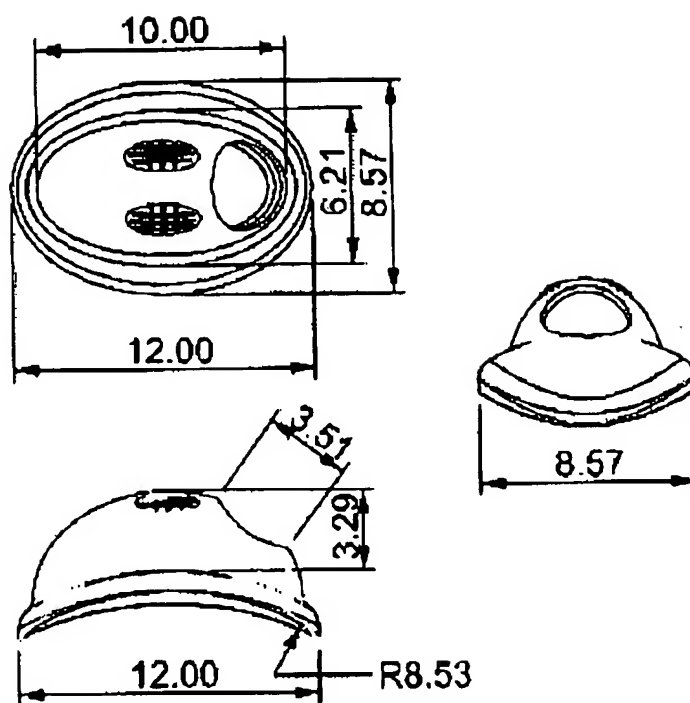


Fig. 22

13

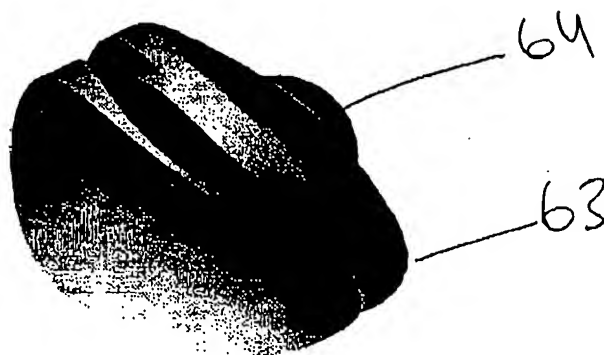


Fig. 23

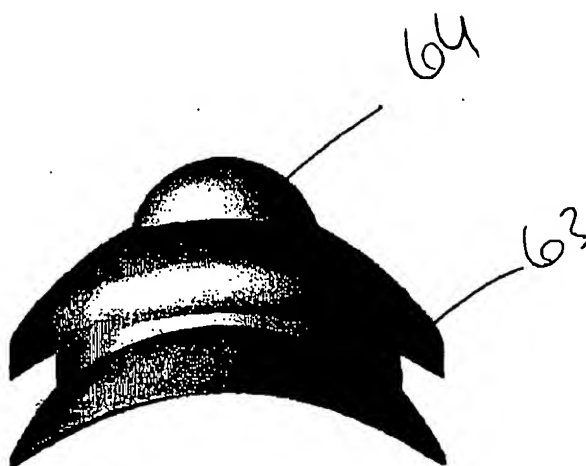


Fig. 24

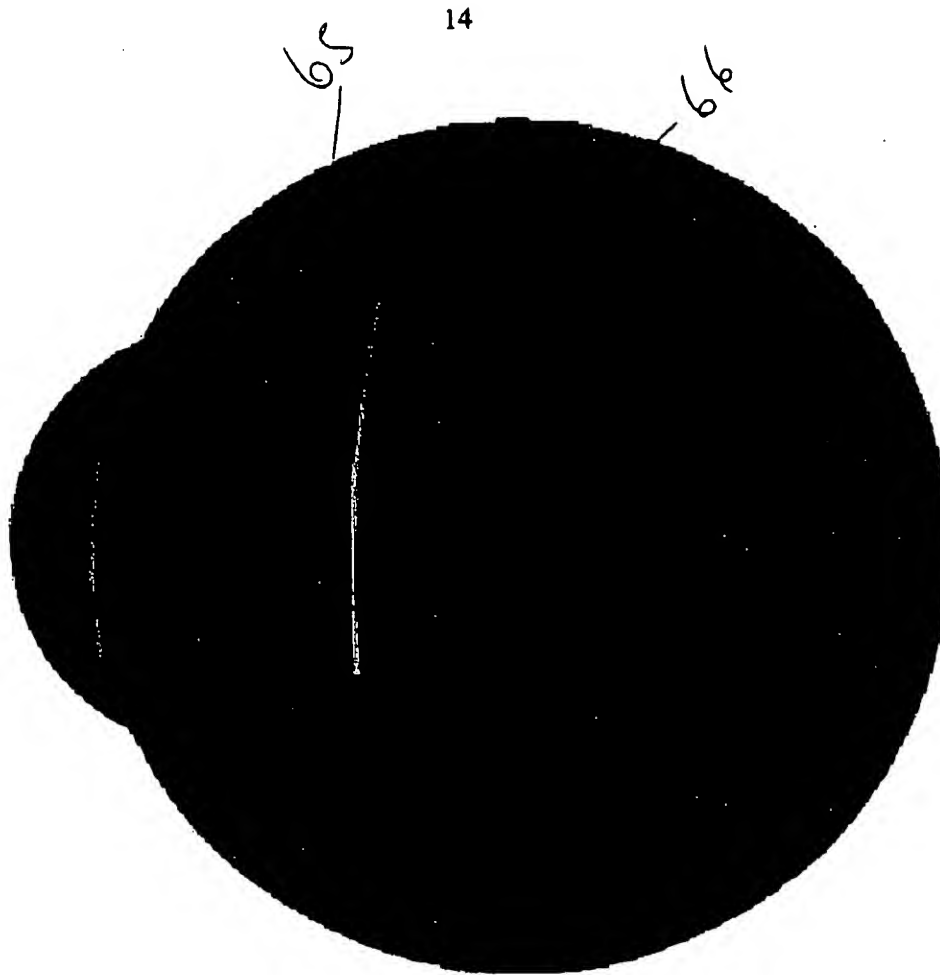


Fig. 25

15

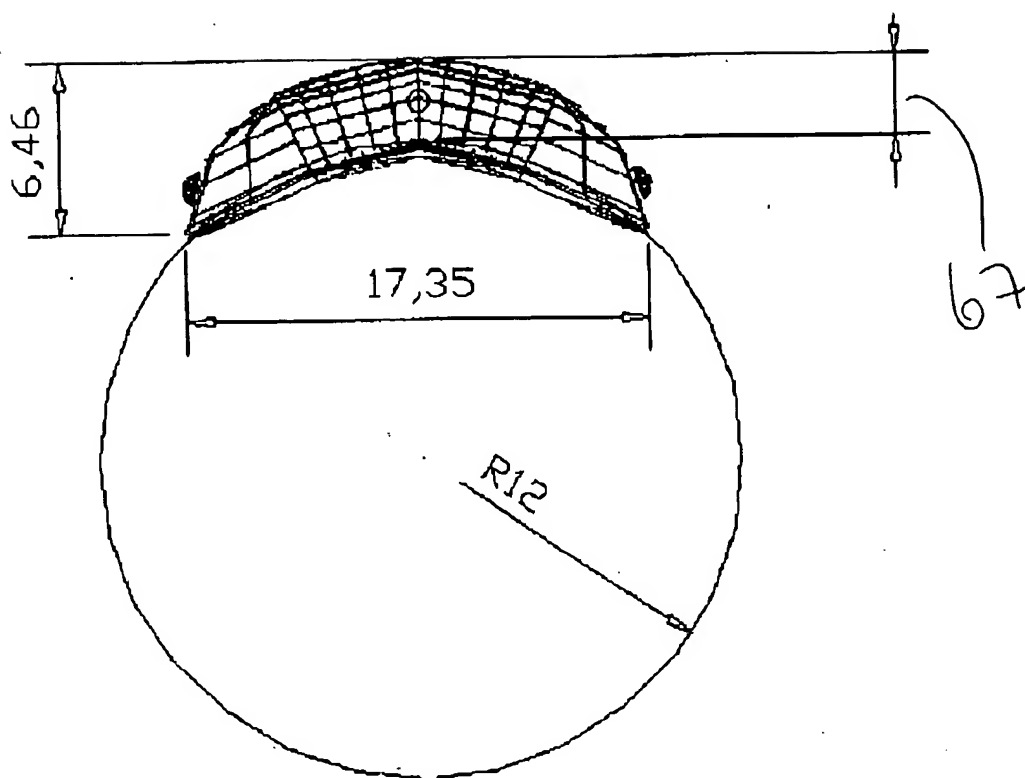


Fig. 26



16

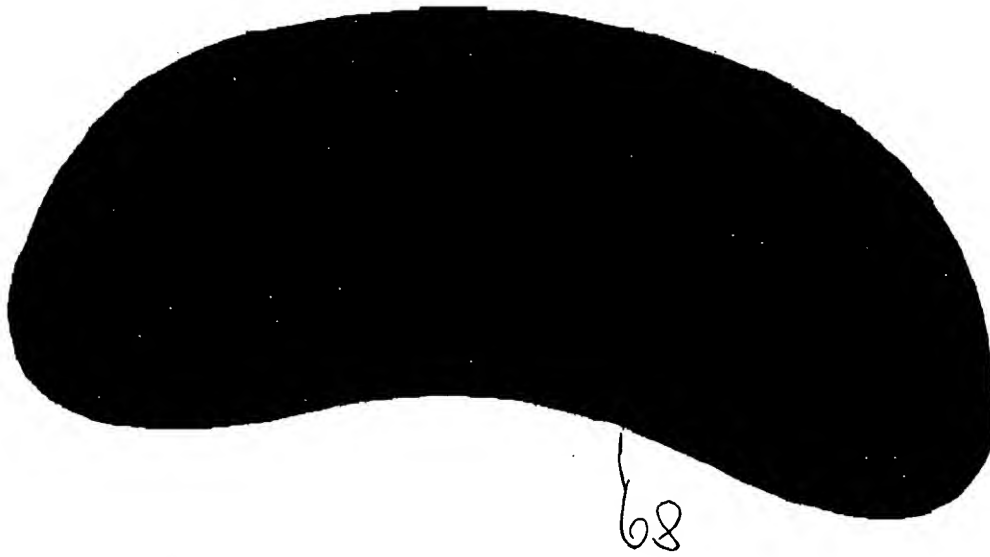


Fig. 27

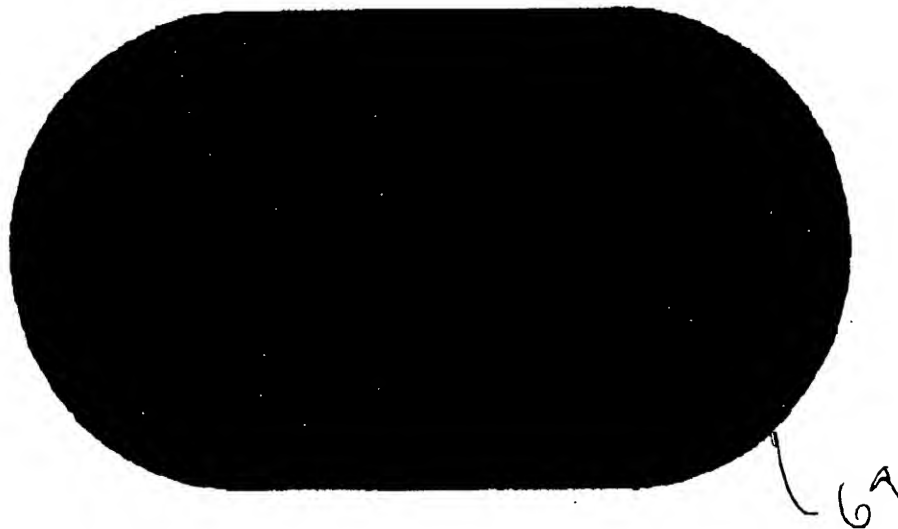


Fig. 28

16

17

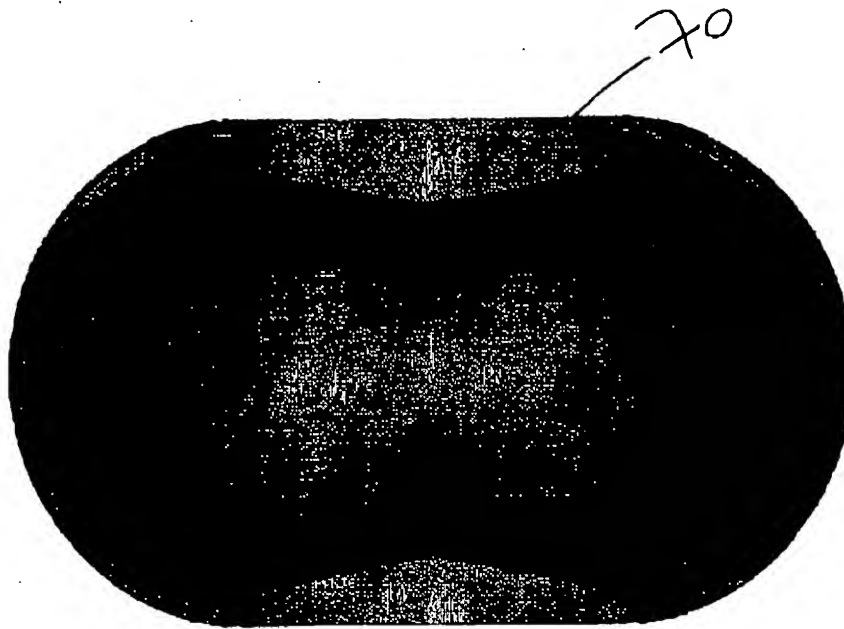


Fig. 29

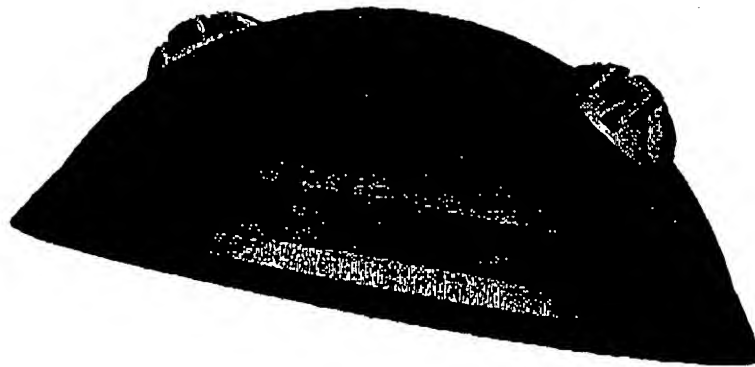


Fig. 30

17



19

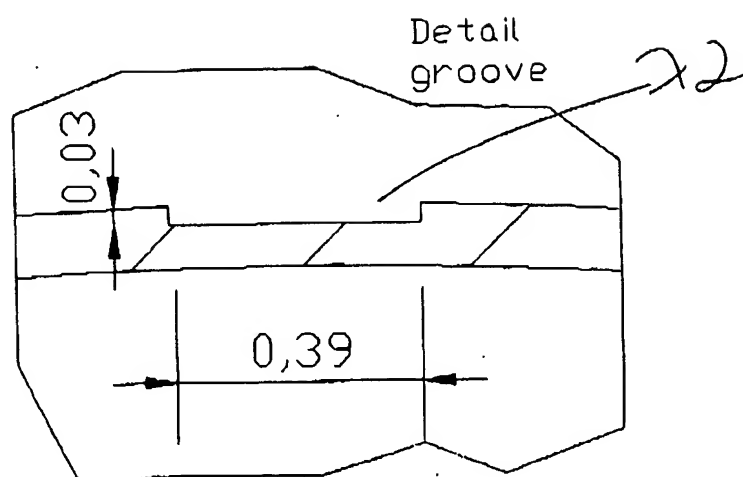


Fig. 33

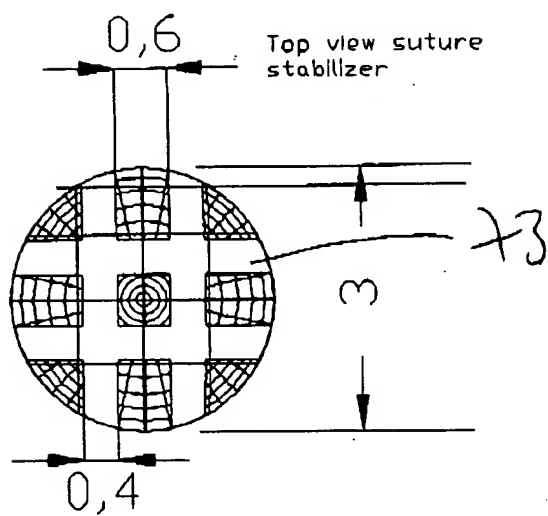


Fig. 34

19

20

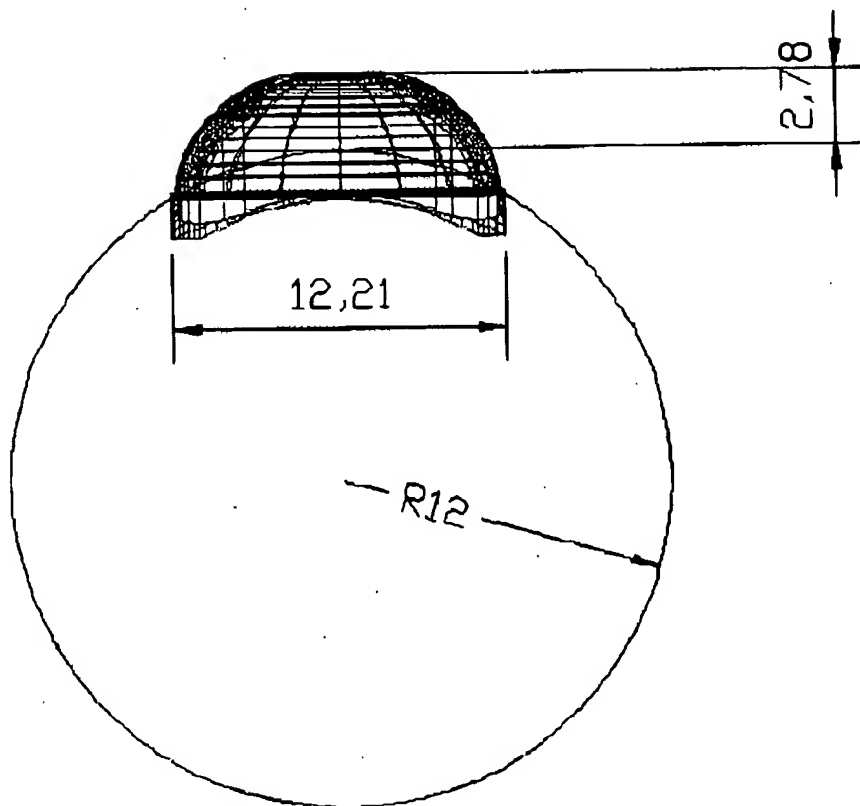


Fig. 35

21

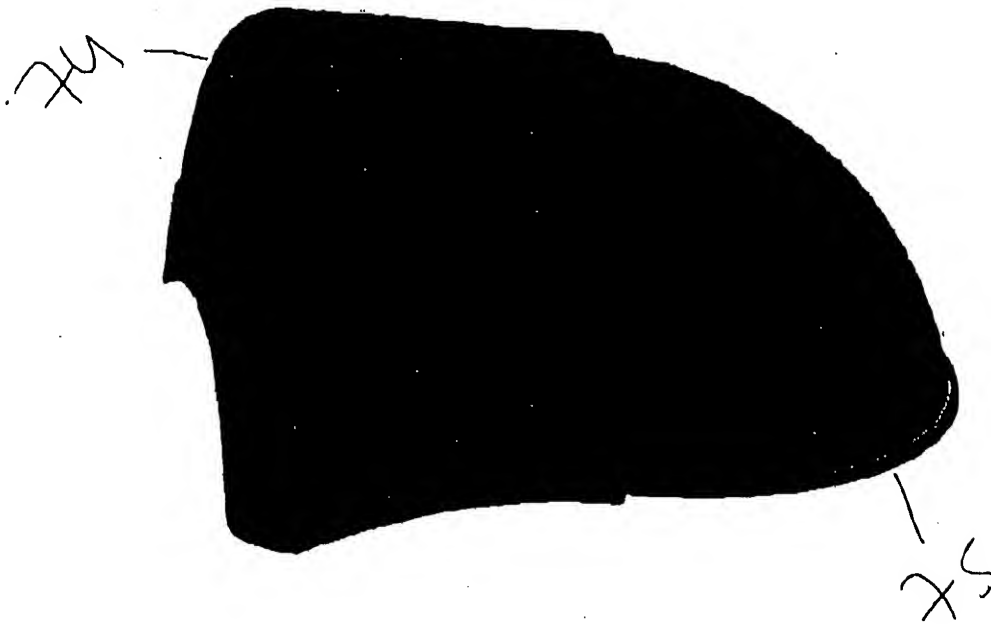


Fig. 36

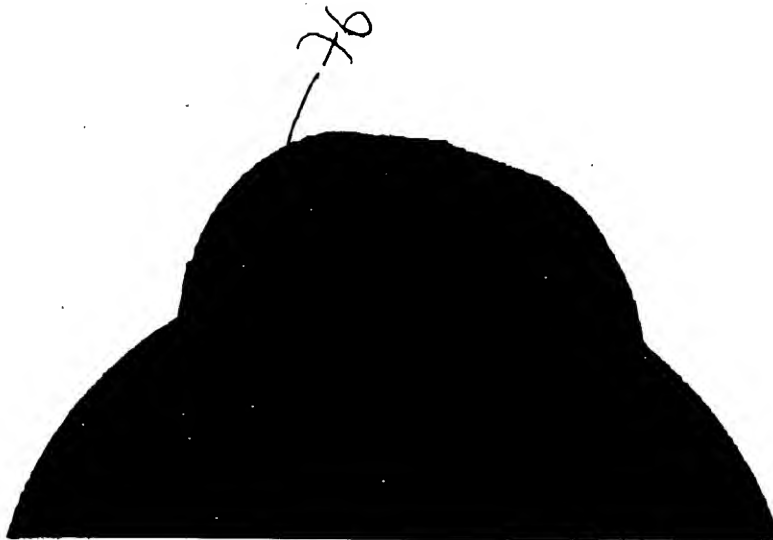


Fig. 37

21

22

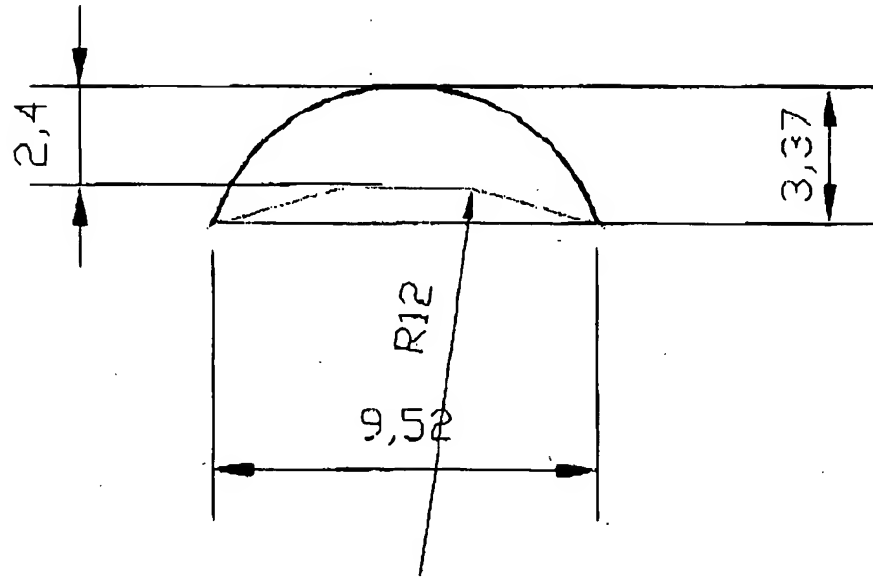


Fig. 38

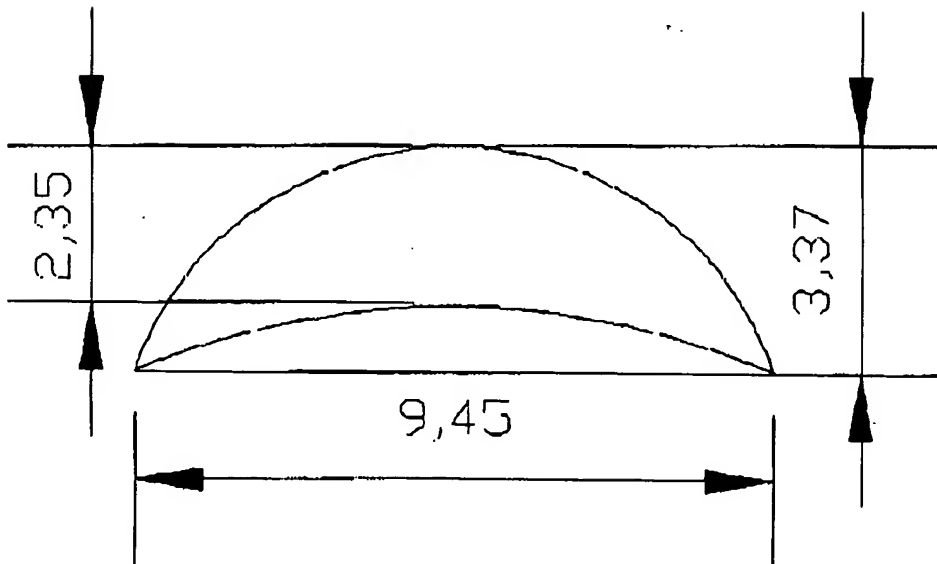


Fig. 39

22

23

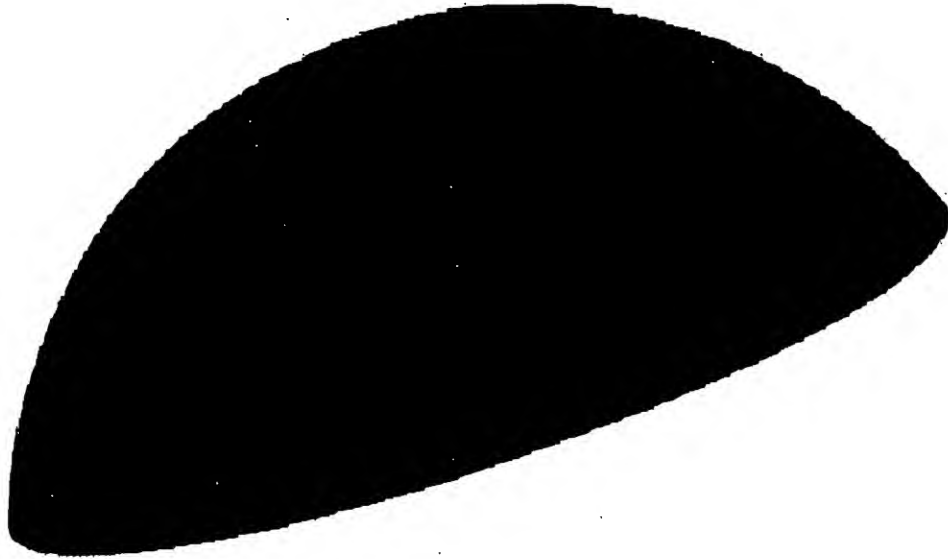


Fig. 40



24

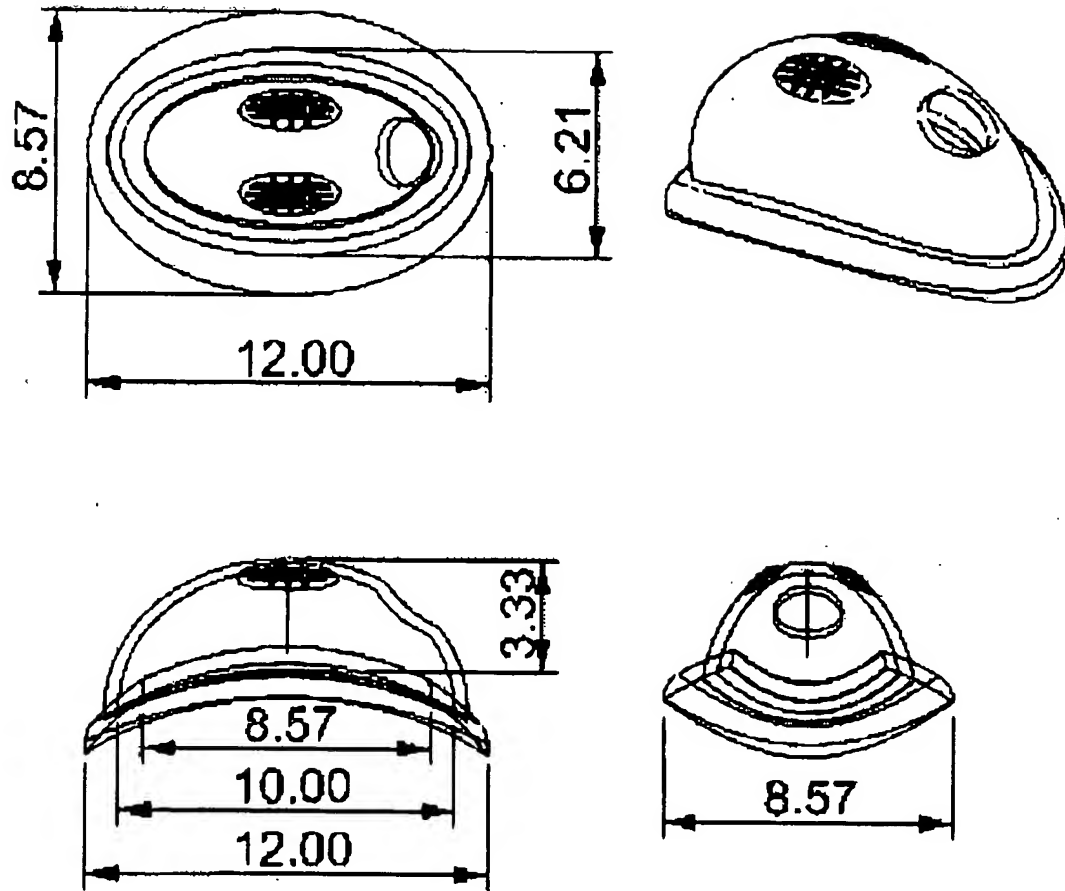


Fig. 41

25

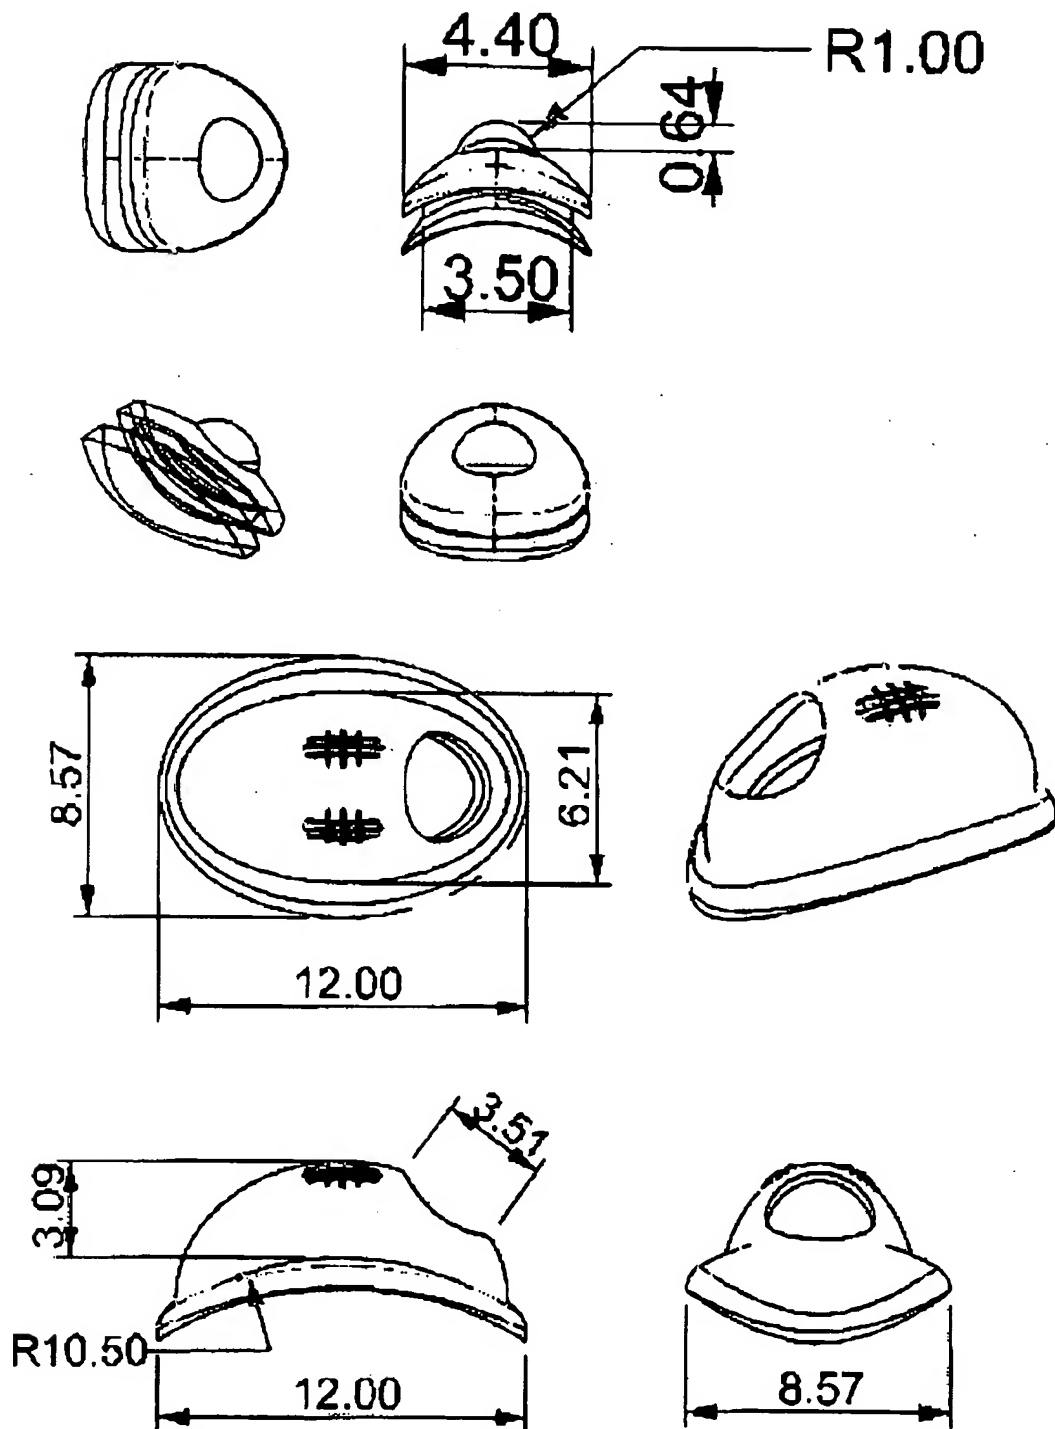


Fig. 42

26

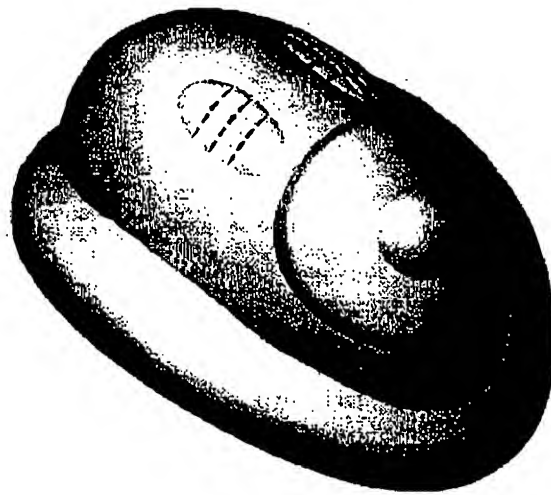


Fig. 43

27

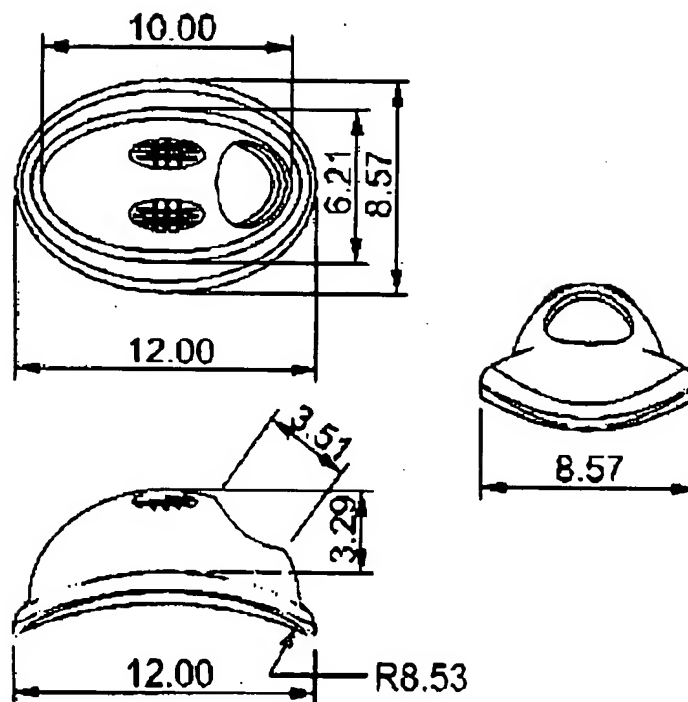


Fig. 44

28

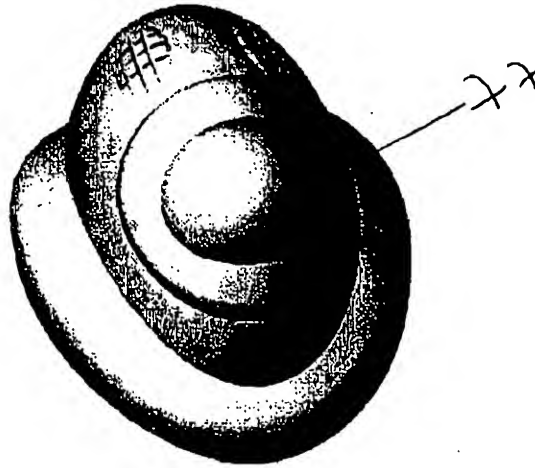


Fig. 45